



International Organization for Migration (IOM)
The UN Migration Agency

Date. 12/05/2021

Bid Bulletin No 3

Supply and Delivery of 10 Modular Clinics and 2 Trucks.

IFB No: 2021/MED/06/MC

Question 1:

kindly define the following

General Medicine - Emergency Clinic

- (i) Line Item 12 - Colour Test – How many plates in need, is it for adults?
- (ii) Line Item 21 - General Instrument Kit-Kindly define what needs to be included
- (iii) Line Item 33 - Sharp Container- Please define the liters
- (iv) Line item 45 - Vital Sign Monitor With 3 Lead Ecg And Respirations- Is it a multiparameter monitor in need
- (v) Line item 50-Diagnostic Set with Sphygmomanometer- What the set needs to include?
- (vi) Line item 51- Is it a waiting chair for patient, please provide more information
- (vii) Line item 54-Refil Antibac Bottles- please provide more information, we cannot comprehend
- (viii) Line item 61- Defibrillator- Please provide more information as there are prices starting from 750€ to 1600€ to 6500€ to 8900 and even more
- (ix) Line item 62- Rescue Bag with Equipment – what equipment need to be included please provide more information
- (x) Line Item 12 - Colour Test – How many plates in need, is it for adults?

Answer 1:

- (i) 2 plates. Yes.
- (ii) 5 Disposable Stapling set - disposable surgical tools.
- (iii) 18.5H X 17.75W X 11.75D Inch 9 Gallon.
- (iv) The necessary indications are:
 - ECG (Electrocardiogram).
 - Breathing rate.
 - SpO2.
 - NIBP (Non Invasible Blood Pressure)
 - Optional indication for temperature.

- (v) The fully equipped diagnostic set shall include one Digital Blood Pressure Monitor, one Otolaryngoscope, one Ophthalmoscope, one Stethoscope, one Oxymeter, one Inhibitor, one Rhinoscope and two Non-Contact Infrared Thermometer.
- (vi) Yes it is for the examination of the patients.
- (vii) Antibacterial hand sanitizer.
- *Desinfection of hands without the use of soap and water.*
 - *Alcohol 70% v/v.*
- (viii) Please note that we cannot disclose any financial information. A mid-range defibrillator will be considered adequate.
- (ix) Rescue Bag with Equipment it is a multi-purpose emergency medical kit filled with medical supplies and equipment in order to better meet the demands of prevalent disaster-related medical issues including infection tools, diagnostics, trauma care and personal protection tools. Each pack shall contain at least Stethoscope, Otolaryngoscope, Sphygmomanometer, different types of Syringes, Bloodstopper, Multi Trauma Dressings, Sterile Conforming Bandages, Sterile Pads, Abdominal Pads, Asherman Chest Seal, Lifesaver CPR Mask, Disposable Airway Kit, Antimicrobial Hand Wipes, Nitrile Gloves, One-use surgical masks, EMI Flexible Splint, Thermal Rescue Blankets, T.A.T. Tourniquet, Adult Nylon Blood Pressure Cuff, Rescuer Knife, EMS Shears (Black), Bandage Scissors (Black), Straight Kelly Forceps (Black), Splinter Forceps (Black), Penlight Black, Starburst Flashlight (Black), Portable oxygen tank, Antecubital lines, Infusion stand, Catheter, Adrenalin shot, Tongue Blades, Hand And Wrist Splint, Antiseptic Wipes, Sodium Chloride 0.9%, 5" X 9" ABD Pad, 8" X 10" ABD Pad, Splint Small 12" X 6", Ambu mask, 5 sizes of Tracheal tubes.
- (x) 2 plates. Yes.

Question 2:


In par. ... page 22 (Purchaser's specifications) you mention that the trucks shall be 4X4 EURO 3 . Kindly note that EURO 3 are now obsolete and the way it is written bidder cannot offer newer EURO class. Kindly re-phrase as "EURO 5 or higher-newer".

Answer 2:

Euro-6 or adequate type of vehicle which will meet the requirements of the current legal framework.

Question 3:

In top of page 23 you mention that Frame length shall be 15.000mm (ie 15m). According to EU and Hellenic Republic / Ministry of Transportation laws and regulations, this **cannot be achieved and type approval cannot be granted**. It needs to be re-phrased as "15m approximately or according to Greek legislation for this type of trucks"

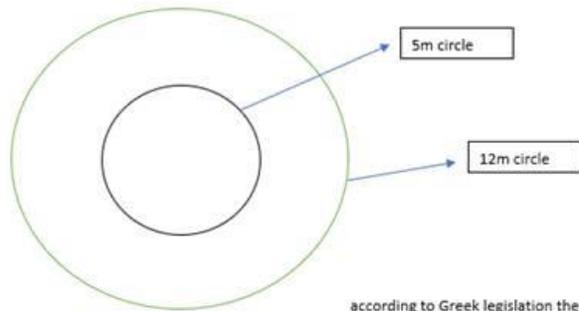

according to Greek legislation the inner circle (5m diameter) and the outer circle 12m diameter the towable trailer shall be moving within the threshold. A 15m length will not get approval except if IOM will issue a relevant particular Ministerial decision.

The max regular (within law limits) type approval max dimensions shall have



Answer 3:

The trailer should be approximately 13,6 m and under no circumstances the trailer with the truck should not be exceeded the specifications defined by the current legislation.

Question 4:

Please confirm that you request ten (10) trailers (clinics) and **each trailer (clinic) to have all particular rooms and all equipment as described in a/a 1 to 8 from pages 25 to 35**. It is noted that room may not be sufficient to include all rooms described.

Answer 4:

We confirm the request of ten (10) trailers (clinics) and each trailer (clinic) to have all particular rooms and all equipment as described in a/a 1 to 8 from pages 25 to 35.

Question 5:

Please note that according to Hellenic Republic / Ministry of Transportation each truck (vehicle) shall have same license plate to the respective trailer (in this case each clinic) in the case it is IX (Ιδιωτικής Χρήσης) . In the case it is ΔΧ (Δημόσιας Χρήσης) special Decree has to be issued by the Ministry. Please note this as in the case that **only 2 trucks are required , they may not be able to carry all 10 towable clinics**.

Answer 5:

Please note that a ΔΧ (Δημόσιας Χρήσης) special Degree will need to be issued.

Question 6:

It is requested 2 tractor trucks with Euro 3 engines, which is not in accordance with the current European regulation, can we propose trucks with engines meeting the Euro 6 standard

Answer 6:

Euro-6 or adequate type of vehicle which will meet the requirements of the current legal framework.

Question 7:

It is requested trailers with a length of 15,000mm which is not in accordance with what is requested on page 25 of the bidding document:

ISO/EU: All trailers must comply with ISO and EU standards for brake lights (air brakes), couplings and any other safety regulations/standards, including UN/ECE regulations. 13, Directive (EU) 2015/719 and 97/27 / EC, Regulations 661/2009 and 1230/2012.

Can we offer trailers with a shorter length that meet the requirements of the above mentioned regulations for category O vehicles?

Answer 7:

The trailer should be approximately 13,6 m and under no circumstances the trailer with the truck should not be exceeded the specifications defined by the current legislation.

Question 8:

Will IOM import the modular clinics, trucks and all medical/non-medical equipment after arrival to Greece for goods delivered from outside of Greece? Or will they issue a notarized proxy letter to authorize the bidder and/or his transport company to import?

Answer 8:

IOM will import the trucks, trailers and the relevant medical equipment after their arrival to Greece.

Question 9:

Will IOM register the modular clinics and trucks themselves or is it expected from the successful bidder

Answer 9:

It is within the responsibility of the vendor.

Question 10:

Will IOM provide exemption letters against any taxes prior to delivering the modular clinics and trucks?

Answer 10:

IOM will import the trucks and trailers and relevant equipment after their arrival to Greece. Following their final delivery to the designated locations by the GoG, the relevant VAT exemption protocols will be issued by the respective Greek Authorities and in turn IOM will submit them to the vendor.

Question 11:

Mandatory emission level for heavy commercial vehicles in Greece is Euro-6. The requested trucks are mentioned to be Euro-3 in Section-III. Will IOM get an exemption for import of the vehicles with Euro-3 emission level

Answer 11:

Euro-6 or adequate type of vehicle which will meet the requirements of the current legal framework.

Question 12:

Does the on-board generator have to comply with the Euro 5 pollution standard, as required by the current European regulations ?

Answer 12:

We confirm that the on-board generator will have to comply with the Euro 5 pollution standard, as required by the current European regulations.

Question 13:

How will the wastewater discharge be done? Once the tank is full, will it be directly discharged to a tank/sewage system or cesspit directly or any intermediate storage is requested?

Answer 13:

In case of sewage system the amount of the wastewater can be discharged directly in this system.

If there is cesspit the wastewater produced from the clinic have to go through chlorination before they be deposited in the cesspit.

Question 14:

Section A article 2.1 states that the bid is open to bidders from eligible countries. Is there any restriction on the Eligible countries? Is a company registered in Republic of Turkey accepted as a source from an eligible country?

Answer 14:

Please be informed that all countries are deemed to be eligible source countries.